
Meril

Obtura™

Vascular Closure Device

Assured Closure. Delivered !

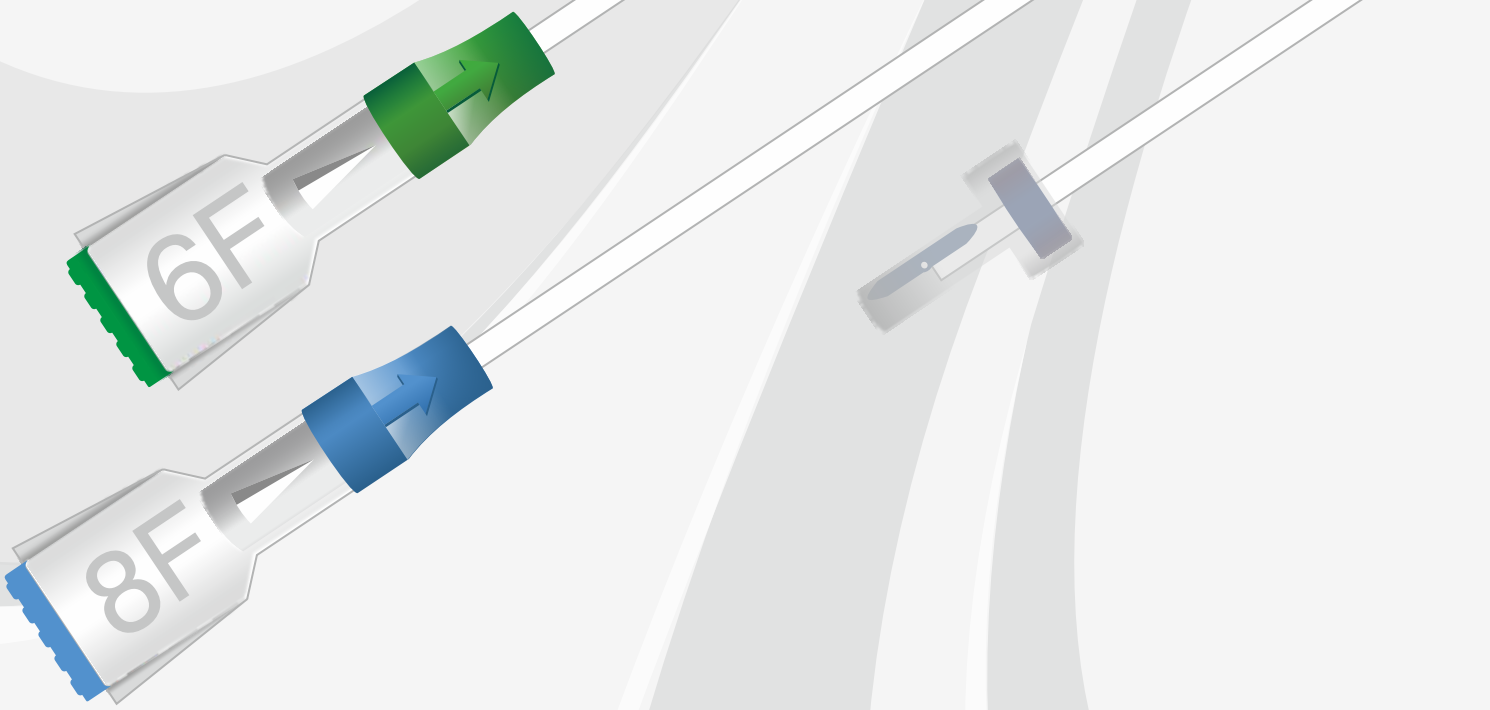

Obtura™

Vascular Closure Device

The Obtura™ Vascular Closure Device is a mechanical closure system which provides an unassailable sealing of the arterial puncture without exchanging Introducer Sheath making it easy to use and providing rapid hemostasis.


- NO exchange of Introducer Sheath
- Less procedural time
- Rapid Hemostasis and less blood loss
- 90 days absorption
- Easy to use Mechanical technique



Device Specifications:

Parameter	Specification
Device Size (F)	6 and 8
Device Total Length (mm)	205
Device Effective Length(mm)	155
Complete Degradation Period (days)	90
Device Size Compatibility	6F device compatible with 6F & 7F Introducer Sheath 8F device compatible with 8F & 9F Introducer Sheath
Introducer Sheath Compatibility	**Medtronic:** InPut Introducer Sheath **Cordis Corporation:** AVANTI™ Introducer Sheath **Terumo Corporation:** PINNACLE Introducer Sheath **Oscor Inc:** Adelante **Merit Medical:** Prelude
Compatible Introducer Sheath Length(cm)	12

Simple Three Step Procedure:

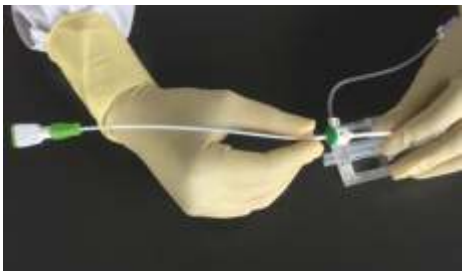

Step 1: Grasp the device at Bypass tube between two fingers like a pen such that size indicator 6F/8F on Hub and Arrow mark on Slider Hub appears upwards.



Step 2: Pull the Hub until the Black Marker appears.



Step 3: Grasping the three components Hub, Slider Hub and Hub of the Introducer Sheath in palm, retract the entire device along with the introducer sheath. Keep the tension on Suture.

Ordering Information:

Reference Number	French Size
OBT6F	6F
OBT8F	8F

Meril Life Sciences Pvt. Ltd.
M1-M2, Meril Park, Survey No 135/2/B & 174/2, Muktanand Marg,
Chala, Vapi - 396 191, Gujarat, India.
T : +91 260 3052 100 F : +91 260 3052 125 E : askinfo@merillife.com W : www.merillife.com

Global Offices:
Meril Turkey | Meril South America | Meril Germany